




Sterilization Indicator



Chemical Indicator

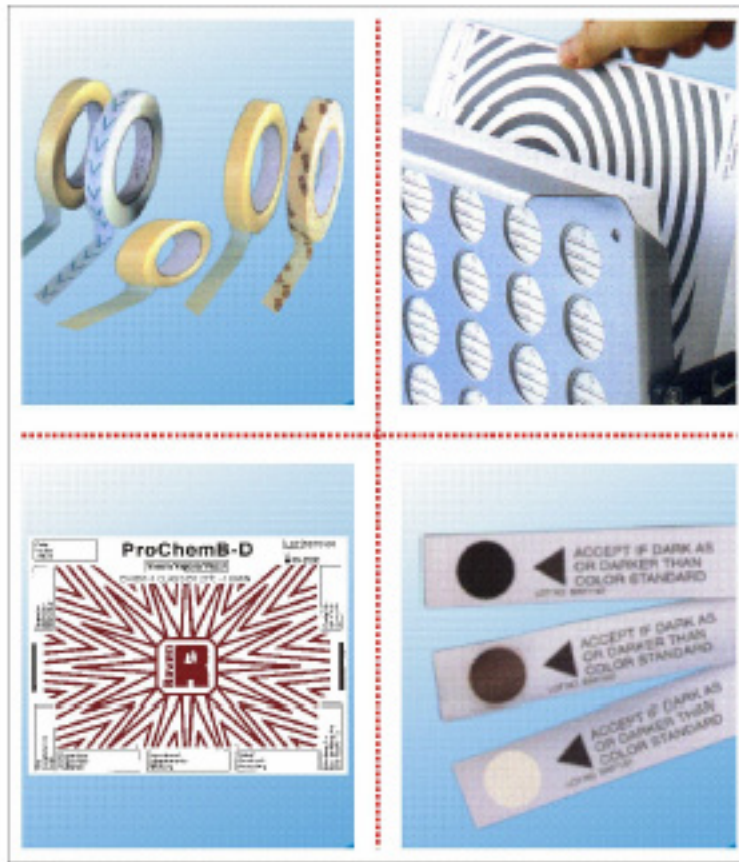

Biological I Indicator



For Routine Monitoring and biological validation of
Steam, ETO, Dry Heat, Gamma & Sterrad®